



IFW

IN THE UNITED STATES PATENT AND TRADEMARK OFFICE

In re Patent Application of

JOHANSSON, R.

Atty. Ref.: 4448-9

Serial No. 10/808,505

TC/A.U.: 3764

Filed: March 25, 2004

Examiner: Not yet assigned

For: AN APPARATUS FOR EVALUATING MANUAL
DEXTERITY

* * * * *

June 17, 2004

Commissioner for Patents
P.O. Box 1450
Alexandria, VA 22313-1450

Sir:

SUBMISSION OF PRIORITY DOCUMENT


It is respectfully requested that this application be given the benefit of the foreign filing date under the provisions of 35 U.S.C. §119 of the following, a certified copy of which is submitted herewith:

<u>Application No.</u>	<u>Country of Origin</u>	<u>Filed</u>
0103238-2	SE	28 September 2001

Respectfully submitted,

NIXON & VANDERHYE P.C.

By: _____

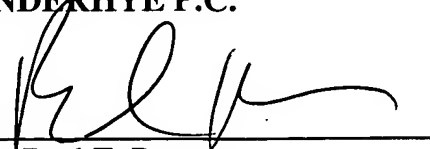
Paul T. Bowen
Reg. No. 38,009

PTB:glf
1100 North Glebe Road, 8th Floor
Arlington, VA 22201-4714
Telephone: (703) 816-4000
Facsimile: (703) 816-4100

PRV

PATENT- OCH REGISTRERINGSVERKET
Patentavdelningen

Intyg Certificate

Härmed intygas att bifogade kopior överensstämmer med de handlingar som ursprungligen ingivits till Patent- och registreringsverket i nedannämnda ansökan.

This is to certify that the annexed is a true copy of the documents as originally filed with the Patent- and Registration Office in connection with the following patent application.

(71) *Sökande* *Roland Sixten Johansson, Umeå SE*
Applicant (s)

(21) *Patentansökningsnummer* *0103238-2*
Patent application number

(86) *Ingivningsdatum* *2001-09-28*
Date of filing

Stockholm, 2004-03-30

För Patent- och registreringsverket
For the Patent- and Registration Office



Hjordis Segerlund

Avgift
Fee *170:-*

AN APPARATUS FOR EVALUATING MANUAL DEXTERITY

The present invention relates to an apparatus for evaluating manual dexterity in humans and in particular to an apparatus for evaluating the manual dexterity of humans with an impaired nervous system and/or musculoskeletal system.

Manual dexterity of humans can provide useful information in relation to their nervous system and/or musculoskeletal system. This information is required for a variety of reasons ranging from pre-operative, post-operative and ongoing assessment of functional abnormalities in patients to prognosis and diagnosis of patients. Additionally, evaluation of manual dexterity can provide valuable information for insurance companies for whom accurate assessment of the recovery of accident victims is vital to prevent against fraudulent claims.

A variety of apparatuses have been manufactured and a number of methods have been devised in order to assist medics and other interested parties with the complex technique of assessing and evaluating manual dexterity in humans. US Patent No. 5,174,154 discloses an isometric force-measuring pinch meter having first and second opposed force-bearing surfaces. An incompressible, nonfluid material is positioned between the first and second surfaces and is capable of building up pressure in response to the application of force to the force-bearing surfaces. A pressure transducer is responsive to the pressure stored in the material for producing an output signal representative of the force. The apparatus is for use with either hand for measuring pinch strength and for ease of application of the fingers and thumb about the apparatus. It also removes any inaccuracies induced by misalignment of the thumb and fingers on the device itself.

US Patent No. 4,674,330 discloses an apparatus for measurement of both the grip strength of a person's hand and the pinch strength of two digits of the hand. The apparatus comprises two parallel grip handles extending at right angles from a third member. The handles are rigidly fixed to the third member and have two pairs of strain gauges to measure the force applied to the handles irrespective of where that force is applied. The ends of the handles terminate in flat portions to be used for measurement of pinch strength. Again, the apparatus is for use with either hand for measuring both grip strength and pinch strength. US Patent No. 4,878,384 discloses a device for evaluating and measuring human sensory perception by measuring muscle force applied against a finger button and displaying a maximum muscle

force. US Patent No. 5,449,002 discloses an apparatus for recording the mechanical pressure applied by a patient recovering from injury or suffering from a disability during routine physical functions such as gripping by the hand. The apparatus utilises a technique known as biofeedback to help patients relearn functions or prevent complications that impede functions.

- 5 German Patent No. DE 4,209,193 discloses an apparatus known as an Ergo graph for measuring the grip of a patients hand in addition to a method for measuring the personality changes in a patient as a result of brain damage suffered by the patient.

- 10 A substantial proportion of nervous system or musculoskeletal impairments are unilateral and therefore a person having such an impairment may have one hand in perfect working order. In order to fully asses the extent of the impairment of the nervous system and/or the musculoskeletal system it is essential to have a set of control data from a fully functional unimpaired hand to compare the data received from a damaged hand with.

- 15 All of the apparatuses and methods dislosed in the patent specifications discussed above are designed to record forces applied by a subject in one direction only. However, manual dexterity and object manipulation is a three dimensional activity and any attempt to evaluate it should take this fact into consideration.

- 20 Clearly there is a need for an improved apparatus and method for quantitatively assessing manual dexterity of a human in order to evaluate the level of impairment of the nervous system and the musculoskeletal system as a result of an accident or as a result of a mental or physical disability.

- 25 Accordingly, there is provided an apparatus for evaluating manual dexterity and object manipulation in humans comprising a means for receiving a hand and a means for measuring and recording omnidirectional forces applied by said hand.

- 30 In one embodiment, the hand receiving means is designed for use by a single hand. In this way, the apparatus can record omnidirectional forces applied by either hand of a person separately. Torques applied by the subject can also be recorded.

In this embodiment, the hand receiving means is detachably mountable about a work surface.

In this embodiment, the hand receiving means includes a handle for receiving a hand and a connecting member for detachably mounting the handle through a flexible joint on said work surface.

- 5 Preferably, the hand receiving means comprises a means for connecting two hands wherein each hand is capable of transmitting a force onto the other hand via the connecting means and the apparatus comprises a means for measuring and recording forces applied by each hand.

- In one aspect of the invention, one person holds the connecting means between both hands.
10 The apparatus allows simultaneous measurement of the capacities of the left and the right hand. Thus, with unilateral impairments the contra lateral (unimpaired) hand will immediately serve as a reference.

- In a further aspect of the invention, the connecting means is held by two people, with each
15 person holding the apparatus by one hand. Beneficially, if one of the people, an experimenter holds the connecting means at one end and the second person, a subject holds the connecting means at the other end, both the experimenters hand and the subjects hand can be evaluated independently.

- 20 Preferably, the connecting means is provided by a hand-held unit. This removes the influence of all variables except gravity and forces applied by subjects holding the hand held unit.

- Preferably, the apparatus further comprises a control unit in communication with the measuring and recording means for recording and analysing forces received by the measuring
25 and recording means. On-line communication between the control unit and the measuring and recording means increases the functionality of the apparatus.

- Ideally, the control unit is in communication with the measuring and recording means telemetrically. This allows the apparatus to take advantage of digital telemetric techniques
30 that are available as silicon chips.

In another embodiment, the control unit and the measuring and recording means are physically connected by electrical cable.

Ideally, the control unit is provided by a computer and a variety of peripheral devices such as speakers and a display screen.

5 Preferably, the computer is configured by a customised control program. The control program is an important feature of the invention providing the apparatus with on-line functionality.

Ideally, the hand-held unit comprises a pair of handles attachable about either end of a joining member wherein the joining member transmits forces between said handles.

10 In one embodiment, the handles are fixed to the joining member.

In another embodiment, the handles are rotatable about the longitudinal axis of the joining member.

15 Ideally, each handle has a pair of grip surfaces for receiving any of the digits of a persons hand. The primary purpose of the apparatus and the associated analysis procedure is the efficient quantitative assessment of the functionality of digits of the subjects hands in terms of force coordination for grasp stability under different grasp loading conditions and the ability to symmetrically apply fingertip forces about opposite grip surfaces of the handles during
20 precision manipulation. Thus, reduction in control of the digits as a result of both impairments in the nervous system and impairments in the musculoskeletal apparatus will be revealed.

In a preferred embodiment, the grip surfaces are provided by longitudinally extending hemi-cylindrical ridges co-axial with the longitudinal axis of the joining member or the connecting
25 member when the handles are mounted on either member. This simplifies assessment of the subject's ability to choose advantageous contact points on the grip surfaces by focusing on their longitudinal dimension. Healthy subjects avoid applying asymmetric forces by opposing digits because it creates unnecessary internal forces within the handles (i.e., uneconomical tangential forces that, in turn, have to be matched by higher grip forces).

30 Preferably, the distance between the grip surfaces is in the range of 10 to 40 millimetres. This allows the apparatus to be used across a wide range of subjects including children and adults having a variety of hand sizes. One area of potential use for the apparatus is thus for following the ontogenetic development of sensorimotor functions. Today, the routine clinical methods

that are used to identify children with sensorimotor impairments are very basic and provide little quantitative evaluation.

Preferably, the handles of the apparatus are equipped with transducers to measure
5 omnidirectional forces generated by the subject at each of the grip surfaces. The transducers permit measurements of coordination between grip forces and tangential forces at each of the two grip surfaces. For each hand, the transducers measure the opposing grip forces applied in directions normal to the length axis of the hand held unit and the load force applied along this axis i.e. push/pull forces. The force tangential to the gripped surfaces at each digit is measured
10 together with torques around the centre of grip force pressure. The total tangential load can be computed based on these measurements.

Ideally, the transducers measure internal forces due to asymmetric applications of the gripping forces produced by opposing digits at each grip surface along with measurements of the
15 points of force pressure centres.

In one embodiment, the handles are attachable about either end of the joining member. This reduces the complexity of the overall apparatus and reduces the number of parts to be designed and manufactured.
20

Preferably, the handles are interchangeable with handles having alternative geometries.

Preferably, handles having parallel, tapered and curved surfaces are used. Obtaining grip stability on different surface geometries requires changes in balance between the grip force and pull/push force applied about the grip surfaces. Thus, sensory information about surface
25 geometry is used to adjust the force balance. Grip stability implies that subjects apply grip forces large enough to avoid accidental slips, while at the same time excessive grip forces are avoided, which naturally may harm the apparatus, injure the hand or cause unnecessary muscle fatigue.

Concerning changes in surface geometry, a powerful variation is implemented by tapered grip surfaces. If the grip surfaces of the handles are tapered towards each other at the end of the handles distal from the joining member or or at the end of the handle distal from the
30 connecting member, healthy subjects apply higher grip forces when they pull on the handle

for maintenance of grip stability in comparison to parallel grip surfaces. With grip surfaces of the handles tapered towards one another at the end of the handles proximate to the joining member or at the end of the handle proximate to the connecting member, stronger grip forces are required when applying push forces.

5

In a preferred embodiment, the geometry of each handle is adjustable by mechanical, electrical or other non-manual means.

10

In one embodiment, a shield is placed between the subject and the handles. This prevents the subject using their vision to adjust the balance required between grip-load force coordination, in particular when working with changes in the geometry of the grip surfaces. It is necessary to avoid visual cues when testing the capacity of the sensibility of the digits to mediate adaptation of the balance between the grip and load forces to variations in the surface geometry.

15

Preferably, both the joining member and the connecting member comprise two sections and a coupling mounted there between.

20

In a preferred embodiment, the two sections are inter-engaged to allow compression and extension of the members along their longitudinal axis in response to push/pull forces applied by a subject and the coupling applies a predetermined biasing force opposing the compression and extension of said members.

25

In a preferred embodiment, the coupling is in communication with the computer and the biasing force applied by the coupling can be momentarily removed in response to a signal from the computer and subsequently reapplied. The coupling between a left and a right section of the members is temporarily broken and subsequently latched. A load rebound occurs when the coupling is latched. This transient load impact triggers automatic gripping force increases based on signals from sensors in the hand in a healthy subject. Results taken from this test can be used to obtain useful information in relation to the nervous system and the musculoskeletal system.

30

Preferably, the computer generates the signal at random times during the test. This will increase the likelihood of obtaining genuine responses from subjects and therefore improve the accuracy of the test.

- 5 Alternatively, the signal is generated by the computer in response to a predetermined time having elapsed from commencement of the test, in response to a certain force applied to the coupling by the subject or in response to a certain distance travelled by the two sections of the members as a result of a force applied by the subject.
- 10 Additionally, the computer generates signals providing information for subjects taking the test.

Preferably, the information includes a demonstration and instructions for the subject taking the test.

15

Ideally, the signals may be audible, visible or tangible. This facilitates people with visual and/or audio deficiencies.

- 20 Preferably, the signals include various pull/push target forces for subjects to aim for. This provides an element of control to the evaluation process and allows an experimenter to set limits for a subject to aim for.

- 25 In one embodiment, the signal is output as a visual display on a screen. This allows for efficient and interactive communication with the subject in terms of providing instructions for the desired actions.

In one embodiment, the screen is a freestanding unit located in front of the subject.

- 30 In a preferred embodiment, the screen is positioned on the joining member between the two handles. This helps to focus the subject's attention entirely on the hand-held unit.

In another embodiment, the screen is positioned on the connecting member between the handle and the workplace.

In another embodiment, the signal is output as an audible signal via speakers. This allows people with impaired vision or blindness to successfully operate the apparatus.

5 Preferably, the computer comprises a means for receiving and storing input forces measured by the transducers.

Ideally, the computer comprises a means for comparing the forces received with a set of control values which are input by the experimenter.

10 Preferably, the computer generates a signal informing the subject that they have successfully completed the current section of the test. This signal is only output after the comparison of current input forces with control values has been carried out and the input forces are acceptable for further processing. This removes the possibility of unsuccessful tests due to unusable data being collected thereby saving time and money.

15

In a particularly preferred embodiment, the computer instantaneously outputs a signal containing the values of current input pull/push forces being received at the grip surfaces and being measured by the transducers to the subject either audibly, visually or tangibly thereby updating the subject on the progress being made.

20

In a still further aspect of the invention, the visual display includes a pre-test demonstration using graphical symbols or characters showing the subject what they are required to do.

25

The invention will now be described with reference to the accompanying drawings and test procedure, which show and outline, by way of example only, one embodiment of an apparatus and method for evaluating manual dexterity in humans in accordance with the invention. In the drawings: -

30

Figure 1 is a schematic drawing showing an elevation view of the apparatus;

Figure 2 is a schematic drawing showing a second embodiment of the apparatus of Figure 1;

Figure 3 is a schematic end view of one handle of the apparatus;

Figure 4 is a schematic elevation view of a hand held unit including a display screen;

Figure 5 is a schematic drawing of a hand held unit showing a coupling;

5 Figure 6 is a schematic drawing of a hand held unit showing a shield;

Figure 7 is a schematic elevation view of a hand held unit having one combination of handles;

10 Figure 8 is a schematic elevation view of a hand held unit having another combination of handles;

Figure 9 is a schematic elevation view of a hand held unit having another combination of handles;

15 Figure 10 is a schematic elevation view of a hand held unit having a still further combination of handles;

20 Figure 11 is a representational graph showing the results of a test conducted using parallel and tapered grip surfaces; and

Figure 12 is a schematic drawing showing one possible visual display to be output on a display screen;

25 Referring to the drawings and initially to Figure 1 there is shown an apparatus for evaluating manual dexterity and object manipulation in humans indicated generally by the reference numeral 1. The apparatus 1 comprises a wall mounted unit 202 and a control unit 3. The control unit 3 is connected to the wall mounted unit 202 by electrical cable 4. The wall mounted unit 202 has a handle 5 and a connecting member 206 for mounting the unit 202 to the wall 100 through a flexible joint. The handle 5 on the left hand side of the unit 202 has parallel grip surfaces 7. Transducers (not shown) are fitted to the grip surfaces 7 and additionally on or about the connection between the handle 5 and the connecting member 206. The control unit 3 comprises a computer 9 having a monitor 10 and speakers (not shown).

30

In Figure 2, the apparatus 1 comprises a hand held unit 2 and a control unit 3. The control unit 3 is connected to the hand held unit 2 by electrical cable 4. The hand held unit 2 comprises a pair of handles 5 and a joining member 6. The handle 5 on the left hand side of the unit 2 has parallel grip surfaces 7 and the handle 5 on the right hand side of the hand held unit 2 has tapered grip surfaces 8. Transducers (not shown) are fitted to the grip surfaces 7 and 8 and additionally on or about the connection between the handles 5 and the joining member 6. The control unit 3 comprises a computer 9 having a monitor 10 and speakers (not shown).

Referring now to Figure 3, there is shown a handle 5 of the hand held unit 2 or wall mounted unit 202. The grip surfaces 12 of the handle 5 are provided by longitudinally extending hemi-cylindrical ridges 11. The ridges 11 are co-axial with the longitudinal axis of the joining member 6 and the connecting member 206 when the handle 5 is mounted on said members 6, 206. The handle 5 is pinched on grip surfaces 12 between a thumb 13 and an index finger 14 of a subject's hand 15. The distance between grip surfaces 12 is typically between 10 mm and 40 mm. In Figure 4, there is shown a hand held unit 31 having a pair of handles 32, a joining member 33 and a display screen 34. The handles 32 have parallel grip surfaces 35 and the display screen 34 is mounted on the joining member 33 of the hand held unit 31.

Referring now to Figure 5, there is shown a hand held unit 41 having a pair of handles 42 and a joining member 43. The joining member 43 has two sections 44 and 45 and a coupling 46 mounted between the two sections 44 and 45. The two sections 44, 45 are inter-engaged to allow compression and extension of the hand held unit 41 about the longitudinal axis of the joining member 43. The coupling 46 is designed to oppose the extension and compression of the hand held unit 41 and is also designed to allow a momentary removal of the opposing force and subsequent latching. A similar coupling (not shown) is incorporated into the connecting member 206 of Figure 1.

Figure 6 shows a further embodiment of the invention wherein a hand held unit 51 has a pair of handles 52, a joining member 53, a display screen 54 and a shield 55. In this example, the shield 55 is mounted between the hand held unit 51 and the display screen 54 in order to prevent a subject from seeing the shape of the handles 52 on the hand held unit 51.

Figures 7 to 10 each show a hand held unit indicated generally by the reference numeral 61. The units 61 each have a joining member 62 and a pair of handles with various geometries. Figure 7 shows a hand held unit 61 with both the left handle and the right handle having parallel grip surfaces 64. Figure 8 shows a hand held unit 61 with the left handle having grip surfaces 74 tapered at 30° to the horizontal and the right handle having parallel grip surfaces 75. Figure 9 shows a hand held unit 61 with the right handle having grip surfaces 84 tapered at 30° to the horizontal and the left handle having parallel grip surfaces 85. Figure 10 shows a hand held unit 61 with both the left handle and the right handle having grip surfaces 94 tapered at an angle of 30° to the horizontal.

10

Referring to the drawings and now to Figure 11 there is shown a representative graph of pull force on the x-axis versus grip force on the y-axis. Line 101 represents a handle with parallel grip surfaces and line 102 represents a handle with tapered grip surfaces. Finally, Figure 12 shows one possible visual display generated by the computer 9 when configured by the control program and output via a display screen 111. An image of an electronic stick-man 112 holding a hand held unit 113 demonstrates what a subject is required to do. The electronic stick-man 112 could also be displayed holding an electronic wall mounted unit (not shown). A visual display of a scale 114 is marked with vertical lines 115 and displays force. This scale 114 shows a subject the zero force marker 116 and the target force marker 117 by highlighting the relevant line 115 along the scale 114. The dot 118 shows the current force. A target for maximum pull force 119 is located at the right end of the scale.

In use, a subject or an examiner starts a test by striking any key on a keyboard of the computer 9. This initiates the demonstration on the display screen 34, 54, 111 or initiates an audible demonstration. The audible demonstration includes a list of verbal instructions output via speakers connected to the computer 9 and is useful for a subject with impaired vision or blindness. When a visual demonstration is used, a pull or push prompt is displayed on the computer screen 34, 35, 11 and in response the stick man 112 stretches or compresses the electronic hand held unit 113 or electronic wall mounted unit (not shown) in order to show a subject the correct action to take in response to a specific prompt. Within the same display screen 34, 54, 111, the scale 114 shows the effect of the stick man 112 stretching or compressing the electronic units 113 by simultaneously moving the current force marker 118 between the zero force marker 116 and the target force marker 117.

- Once a subject is satisfied with the demonstration, they can proceed with the test by striking any key on the keyboard of the computer 9. The hand held unit 2, 31, 41, 51, 61 or wall mounted unit 202 is held by a subject by the grip surfaces 7, 8, 12, 35, 64, 74, 75, 84, 85 and 94 between digits of their hands. The subject then follows a list of prompts displayed on the display screen 34, 54, 111 or a list of verbal instructions output via speakers which are connected to the computer 9. The display also includes the scale 114 which shows the effect of the subject stretching or compressing the hand held unit 2, 31, 41, 51, 61 or wall mounted unit 202 by simultaneously moving the current force marker 118 between the zero force marker 116 and the target force marker 117. The visual display may also include a prompt for the subject to maintain the target force for a predetermined period of time. Once the target force has been attained, the computer 9 monitors the quality of the data received from the transducers (not shown) comparing it with control data. The computer 9 outputs a signal to the display screen 34, 54, 111 informing the subject to release the applied force if the data received is acceptable. Alternatively, these prompts can be output via the speakers. The subject follows the audible or visual instructions until completion of the test. In order to prevent the subject using their vision to alter grip-push/pull force co-ordination a shield 55 is placed between the hand held unit 2, 31, 41, 51, 61 or wall mounted unit 202 and the subject for certain parts of the test.
- The hand held unit 2, 31, 41, 51, 61 is grasped bimanually and the wall mounted unit 202 is grasped by a single hand and manipulated according to a pre-defined (standardized) protocol. An automated test protocol combined with automated data analysis allows efficient assessment of the subject's manual status based on the data obtained from the force/torque transducers of units 2, 31, 41, 51, 61 or 202.
- There now follows a detailed description of an example of a test protocol and data analysis.
1. The subject familiarizes themselves with the apparatus 1 by doing a few ramp-and-hold pull forces and push forces to certain target forces (e.g. + 4 Newtons (N), -4N). Before the action, the task is demonstrated on the display screen 34, 54, 111 by the icon stickman 112 performing the task. The subject's task is to copy the demonstration.

2. The subject performs a series of ramp-and-hold pull forces of different magnitudes according to the predetermined protocol (e.g., 1, 4, 2, 8 Newtons (N)) three times followed by a series of push forces (e.g. 4, 4, 4 N). These tests are repeated for the different geometric configurations of the handles, shown in the drawings. Quality control of the data occurs on-line and is dependent upon the subject maintaining the target push/pull force (within a predefined tolerance) for two seconds. In response to successful completion of the task by the subject, the target marker 117 on the display screen 34, 54, 111 is turned off. An audible signal indicating that this section of the test has been successfully completed could also be generated.

10

Analysis: The computer 9 configured by the control program automatically reads and stores the measured variables during a 2 second epoch while the subject maintains the target force. The coordination between grip force and the load at each hand (and at the level of the individual's digits) is automatically analyzed. The subject's capacity to scale the grip force with the load force and to adjust the balance between the grip force and load with changes in geometry of grip surfaces 7, 8, 12, 35, 64, 74, 75, 84, 85 and 94 is assessed for each hand.

15

3. The subject makes sinusoidal pull forces at different frequencies. The amplitude (e.g. 4N with approximately +/-20% tolerance) is guided by the display screen 34, 54, 111. A metronome sound guides the pace. The frequency range to be explored is 0.5 - 3 Hz. Again, quality control of the data occurs on-line. Before changing to the next frequency, a certain number of cycles with an accepted amplitude and frequency are collected. (The grip surfaces 7, 12, 35, 64, 75, 85 are parallel on all handles.)

20

25 Analysis: The phase between grip force and the load is analyzed; normally there is no phase lag, which indicates that the grip force predicts adequately the self-generated load forces (for grip stability). The depth of grip force modulation is assessed as a function of frequency; normally there is a steep decrease in the modulation with increased frequency, starting at about 1.5 - 2 Hz.

30

4. The subject makes sinusoidal pull-push forces at different frequencies (0.5 - 1.5 Hz) and at constant push-pull amplitudes (e.g. -4N(push) to +4N (pull)). (The grip surfaces 7, 12, 35, 64, 75, 85 are parallel on all handles.) In this task, the absolute value of the tangential load increases and decreases with twice the frequency of the sinusoidal

load. Normal subjects respond to this "frequency doubling" by generating two grip force increases per load cycle i.e. the grip force predicts the actual load although it does not match the frequency of the load cycles.

- 5 Analysis: The phase between grip force and the absolute value of the load and the depth of grip force modulation is analyzed (cf. above). This analysis assesses the subject's ability to generalize the directional consequences of self-generated fingertip loads in terms of grip force requirements (and thus grip force predictions).
- 10 5. The subject produces their maximum bimanual pull force. Normally, a subjects right hand is stronger than their left- yet subjects never allow the left hand to slip off the unit 2, 31, 41, 51, 61 during bimanual operations because the knowledge of their musculoskeletal system is incorporated as a control constraint in the neural networks of the brain. To assess asymmetries of force generating capacity by the two hands, the
- 15 maximum grip force is assessed for each hand separately.
- 20 6. Finally, by imposing the transient load impact at a few unpredictable points during the test protocol numbered 2 (see above) the reflex status of the reactive grip force control of the two hands is assessed. Normally, with two healthy hands, the load impact triggers automatic grip force increases at both hands with similar amplitudes and onset latencies.

The results of the tests provided the following information.

Impairment of sensory functions of the digits is reflected in:

- 25 1. A weakened or lost capacity of the impaired hand to adjust the balance between the grip forces and the load forces in response to changes in geometry of the grip surfaces 7, 8, 12, 35, 64, 74, 75, 84, 85 and 94.
- 30 2. With sensory impairment of one hand, the accompanying healthy hand also controls the grip-load force coordination of the numb hand. Likewise, the healthy hand uses strategies that reflect constraints imposed by the impaired hand during bimanual actions.

3. An impaired hand generates increased internal forces upon the hand held unit 2, 31, 41, 51, 61 or 202 due to asymmetric grip force applications at the opposing grip surfaces 7, 8, 12, 35, 64, 74, 75, 84, 85 and 94. This causes unnecessary/uneconomical load of the grasp.

Impairment of predictive control of grip forces is reflected in:

- 5 1. A temporal mismatch between the grip and load force changes and is revealed during the test with sinusoidal load changes.
2. A reduced modulation of grip forces with load force changes compared to healthy conditions.

Impairment of reactive control of grip forces is reflected in:

- 10 One or several of the following items revealed impaired reactive grip force control: (1-) No response to the transient load impact. (2) A prolonged onset latency of the reactive grip force increases. (3) Smaller amplitudes than normal of the reactive grip force increases. With unilateral impairments, asymmetries between the hands in these respects are important.

- 15 Impairment of the brain's proprioceptive knowledge:

With impaired proprioceptive knowledge concerning one diseased hand the healthy contralateral hand shows incompetence in controlling its actions based on constraints imposed by the diseased hand during bimanual tasks. Impaired proprioceptive knowledge is assessed in the present protocol by an inability of the healthy hand to limit the application of pull force to the hand-held unit as to match the capacity of the companion diseased hand. This is critically revealed during the test of maximum voluntary bimanual pull along the hand-held unit 2, 31, 41, 51, 61. With proprioceptive knowledge the hand-held unit 2, 31, 41, 51, 61 does not slip at the diseased hand, whereas with loss of proprioceptive knowledge the unit 2, 31, 41, 51, 61 slips from the subjects grip.

25

30

CLAIMS

- 5 1. An apparatus (1) for evaluating manual dexterity and object manipulation in humans comprising a means for receiving a hand and a means for measuring and recording omnidirectional forces applied by said hand.
2. An apparatus (1) as claimed in claim 1, wherein the hand receiving means is designed for use by a single hand.
- 10 3. An apparatus (1) as claimed in any preceding claim, wherein the hand receiving means is detachably mountable about a work surface.
- 15 4. An apparatus (1) as claimed in any preceding claim, wherein the hand receiving means includes a handle (5) for receiving a hand and a connecting member (206) for detachably mounting the handle (5) on said work surface through a flexible joint.
- 20 5. An apparatus (1) as claimed in claim 1, wherein the hand receiving means comprises a means for connecting two hands wherein each hand is capable of transmitting a force onto the other hand via the connecting means and the apparatus (1) comprises a means for measuring and recording forces applied by each hand.
- 25 6. An apparatus (1) as claimed in claim 5, wherein one person holds the connecting means between both hands.
7. An apparatus (1) as claimed in claim 5, wherein the connecting means is held by two people, with each person holding the apparatus (1) by one hand.
- 30 8. An apparatus (1) as claimed in any of claims 5 to 7, wherein the connecting means is provided by a hand-held unit (2, 31, 41, 51, 61).
9. An apparatus (1) as claimed in any preceding claim, wherein the apparatus (1) further comprises a control unit (3) in communication with the measuring and recording means for recording and analysing forces received by the measuring and recording means.

10. An apparatus (1) as claimed in claim 9, wherein the control unit (3) is in communication with the measuring and recording means telemetrically.
- 5 11. An apparatus (1) as claimed in claim 9, wherein the control unit (3) is in communication with the measuring and recording means by electrical cable (4).
12. An apparatus (1) as claimed in any of claims 9 to 11, wherein the control unit (3) is provided by a computer (9) and a variety of peripheral devices such as speakers and a display screen (10).
- 10 13. An apparatus (1) as claimed in claim 12, wherein the computer (9) is configured by a customised control program.
- 15 14. An apparatus (1) as claimed in any of claims 8 to 13, wherein the hand-held unit (2, 31, 41, 51, 61) comprises a pair of handles (5) attachable about either end of a joining member (6) and in use the joining member (6) transmits forces between said handles (5).
- 20 15. An apparatus (1) as claimed in claim 14, wherein the handles (5) are fixed to the joining member (6).
16. An apparatus (1) as claimed in claim 14, wherein the handles (5) are rotatable about the longitudinal axis of the joining member (6).
- 25 17. An apparatus (1) as claimed in any of claims 14 and 16, wherein transducers are fitted between the handles (5) and the joining member (6) in order to measure the torque applied by the subject to each handle (5) of the hand-held unit (2, 31, 41, 51, 61).
- 30 18. An apparatus (1) as claimed in any of claims 14 to 17, wherein each handle (5) has a pair of grip surfaces (7, 8, 12, 35, 64, 74, 75, 84, 85, 94) for receiving any of the digits of a person's hand.

19. An apparatus (1) as claimed in claim 18, wherein the grip surfaces (7, 8, 12, 35, 64, 74, 75, 84, 85, 94) are provided by longitudinally extending hemi-cylindrical ridges (11) co-axial with the longitudinal axis of the joining member (6) or the connecting member (206) when the handles (5) are mounted on either member.
20. An apparatus (1) as claimed in claim 18 and claim 19, wherein the distance between the grip surfaces (7, 8, 12, 35, 64, 74, 75, 84, 85, 94) is in the range of 10 to 40 millimetres.
21. An apparatus (1) as claimed in any of claims 14 to 20, wherein the handles (5) of the apparatus (1) are equipped with transducers to measure omnidirectional forces generated by the subject at each of the grip surfaces (7, 8, 12, 35, 64, 74, 75, 84, 85, 94).
22. An apparatus (1) as claimed in claim 17, wherein the transducers measure internal forces due to asymmetric applications of the gripping forces produced by opposing digits at each grip surface (7, 8, 12, 35, 64, 74, 75, 84, 85, 94) along with measurements of the points of force pressure centres.
23. An apparatus (1) as claimed in any of claims 14 to 22, wherein the handles (5) are attachable about either end of the joining member (6).
24. An apparatus (1) as claimed in any of claims 14 to 23, wherein the handles (5) are interchangeable with handles having alternative geometries.
25. An apparatus (1) as claimed in any of claims 14 to 24, wherein the handles (5) have parallel, tapered or curved surfaces.
26. An apparatus (1) as claimed in any of claims 14 to 25, wherein the geometry of each handle (5) is adjustable by mechanical, electrical or other non-manual means.
27. An apparatus (1) as claimed in any of claims 14 to 26, wherein a shield (55) is placed between the subject and the handles (5).

28. An apparatus (1) as claimed in any of claims 4 and claims 14 to 27, wherein the joining member (6) and the connecting member (206) comprise two sections (44, 45) and a coupling (46) mounted between the sections.
- 5 29. An apparatus (1) as claimed in claim 28, wherein the two sections are inter-engaged to allow compression and extension of the members along their longitudinal axis in response to push/pull forces applied by a subject and the coupling applies a predetermined biasing force opposing the compression and extension of said members.
- 10 30. An apparatus (1) as claimed in claims 28 and 29, wherein the coupling (46) is in communication with the computer (9) and the biasing force applied by the coupling can be momentarily removed in response to a signal from the computer and subsequently reapplied.
- 15 31. An apparatus (1) as claimed in claim 30, wherein the computer (9) generates the signal at random times during the test.
- 20 32. An apparatus (1) as claimed in claims 30 and 31, wherein the signal is generated by the computer (9) in response to a predetermined time having elapsed from commencement of the test, in response to a certain force applied to the coupling by the subject or in response to a certain distance travelled by the two sections of either member as a result of a force applied by the subject.
- 25 33. An apparatus (1) as claimed in any of claims 12 to 32, wherein the computer (9) generates signals providing information for subjects taking the test.
- 30 34. An apparatus (1) as claimed in claim 33, wherein the information includes a demonstration and instructions for the subject taking the test.
- 35 35. An apparatus (1) as claimed in any of claims 33 and 34, wherein the signals may be audible, visible or tangible.
36. An apparatus (1) as claimed in any of claims 33 to 35, wherein the signals include various push/pull target forces for subjects to aim for.

37. An apparatus (1) as claimed in any of claims 33 to 36, wherein the signals are output as a visual display on a screen (34, 54, 111).
- 5 38. An apparatus (1) as claimed in any of claims 33 to 36, wherein the signal is output as an audible signal via speakers.
39. An apparatus (1) as claimed in claim 37, wherein, the screen (34, 54, 111) is a freestanding unit located in front of the person.
- 10 40. An apparatus (1) as claimed in claim 37, wherein the screen is mounted on the joining member between the two handles.
41. An apparatus (1) as claimed in claim 37, wherein the screen is mounted on the connecting member between the handle and the workplace.
- 15 42. An apparatus (1) as claimed in any of claims 12 to 41, wherein the computer (9) comprises a means for receiving and storing input forces measured by the transducers.
- 20 43. An apparatus (1) as claimed in any of claims 12 to 42, wherein the computer (9) comprises a means for comparing the forces received with a set of control values which are input by a healthy subject.
- 25 44. An apparatus (1) as claimed in any of claims 12 to 43, wherein the computer generates a signal informing the person that they have successfully completed the current section of the test.
- 30 45. An apparatus (1) as claimed in any of claims 12 to 44, wherein the computer instantaneously outputs a signal to the subject either audibly, visually or tangibly containing the values of current input push/pull forces being received at the grip surfaces and being measured by the transducers thereby updating the subject on the progress being made.

46. An apparatus (1) as claimed in any of claims 37 to 45, wherein the visual display includes a pre-test demonstration using graphical symbols or characters showing the subject what they are required to do.

1
2
3
4
5
6
7
8
9
10

ABSTRACT

The present invention relates to an apparatus (1) for evaluating manual dexterity in humans and in particular to an apparatus (1) for evaluating the manual dexterity of humans with an
5 impaired nervous system and/or musculoskeletal system. Manual dexterity and object manipulation is a three dimensional activity and any attempt to evaluate it should take this fact into consideration. The present invention provides an apparatus (1) for evaluating manual dexterity and object manipulation in humans comprising a means for receiving a hand and a means for measuring and recording omnidirectional forces applied by said hand. Additionally,
10 a means for connecting two hands wherein each hand is capable of transmitting a force onto the other hand via the connecting means is provided and the apparatus comprises a means for measuring and recording forces applied by each hand.

(FIGURE 2)

11
12
13
14
15
16
17
18
19
20
21
22
23
24
25
26
27
28
29
30
31
32
33
34
35
36
37
38
39
40
41
42
43
44
45
46
47
48
49
50
51
52
53
54
55
56
57
58
59
60
61
62
63
64
65
66
67
68
69
70
71
72
73
74
75
76
77
78
79
80
81
82
83
84
85
86
87
88
89
90
91
92
93
94
95
96
97
98
99
100
101
102
103
104
105
106
107
108
109
110
111
112
113
114
115
116
117
118
119
120
121
122
123
124
125
126
127
128
129
130
131
132
133
134
135
136
137
138
139
140
141
142
143
144
145
146
147
148
149
150
151
152
153
154
155
156
157
158
159
160
161
162
163
164
165
166
167
168
169
170
171
172
173
174
175
176
177
178
179
180
181
182
183
184
185
186
187
188
189
190
191
192
193
194
195
196
197
198
199
200
201
202
203
204
205
206
207
208
209
210
211
212
213
214
215
216
217
218
219
220
221
222
223
224
225
226
227
228
229
230
231
232
233
234
235
236
237
238
239
240
241
242
243
244
245
246
247
248
249
250
251
252
253
254
255
256
257
258
259
260
261
262
263
264
265
266
267
268
269
270
271
272
273
274
275
276
277
278
279
280
281
282
283
284
285
286
287
288
289
290
291
292
293
294
295
296
297
298
299
300
301
302
303
304
305
306
307
308
309
310
311
312
313
314
315
316
317
318
319
320
321
322
323
324
325
326
327
328
329
330
331
332
333
334
335
336
337
338
339
340
341
342
343
344
345
346
347
348
349
350
351
352
353
354
355
356
357
358
359
360
361
362
363
364
365
366
367
368
369
370
371
372
373
374
375
376
377
378
379
380
381
382
383
384
385
386
387
388
389
390
391
392
393
394
395
396
397
398
399
400
401
402
403
404
405
406
407
408
409
410
411
412
413
414
415
416
417
418
419
420
421
422
423
424
425
426
427
428
429
430
431
432
433
434
435
436
437
438
439
440
441
442
443
444
445
446
447
448
449
450
451
452
453
454
455
456
457
458
459
460
461
462
463
464
465
466
467
468
469
470
471
472
473
474
475
476
477
478
479
480
481
482
483
484
485
486
487
488
489
490
491
492
493
494
495
496
497
498
499
500
501
502
503
504
505
506
507
508
509
510
511
512
513
514
515
516
517
518
519
520
521
522
523
524
525
526
527
528
529
530
531
532
533
534
535
536
537
538
539
540
541
542
543
544
545
546
547
548
549
550
551
552
553
554
555
556
557
558
559
560
561
562
563
564
565
566
567
568
569
570
571
572
573
574
575
576
577
578
579
580
581
582
583
584
585
586
587
588
589
590
591
592
593
594
595
596
597
598
599
600
601
602
603
604
605
606
607
608
609
610
611
612
613
614
615
616
617
618
619
620
621
622
623
624
625
626
627
628
629
630
631
632
633
634
635
636
637
638
639
640
641
642
643
644
645
646
647
648
649
650
651
652
653
654
655
656
657
658
659
660
661
662
663
664
665
666
667
668
669
670
671
672
673
674
675
676
677
678
679
680
681
682
683
684
685
686
687
688
689
690
691
692
693
694
695
696
697
698
699
700
701
702
703
704
705
706
707
708
709
710
711
712
713
714
715
716
717
718
719
720
721
722
723
724
725
726
727
728
729
730
731
732
733
734
735
736
737
738
739
740
741
742
743
744
745
746
747
748
749
750
751
752
753
754
755
756
757
758
759
760
761
762
763
764
765
766
767
768
769
770
771
772
773
774
775
776
777
778
779
780
781
782
783
784
785
786
787
788
789
790
791
792
793
794
795
796
797
798
799
800
801
802
803
804
805
806
807
808
809
810
811
812
813
814
815
816
817
818
819
820
821
822
823
824
825
826
827
828
829
830
831
832
833
834
835
836
837
838
839
840
841
842
843
844
845
846
847
848
849
850
851
852
853
854
855
856
857
858
859
860
861
862
863
864
865
866
867
868
869
870
871
872
873
874
875
876
877
878
879
880
881
882
883
884
885
886
887
888
889
890
891
892
893
894
895
896
897
898
899
900
901
902
903
904
905
906
907
908
909
910
911
912
913
914
915
916
917
918
919
920
921
922
923
924
925
926
927
928
929
930
931
932
933
934
935
936
937
938
939
940
941
942
943
944
945
946
947
948
949
950
951
952
953
954
955
956
957
958
959
960
961
962
963
964
965
966
967
968
969
970
971
972
973
974
975
976
977
978
979
980
981
982
983
984
985
986
987
988
989
990
991
992
993
994
995
996
997
998
999
1000
1001
1002
1003
1004
1005
1006
1007
1008
1009
1010
1011
1012
1013
1014
1015
1016
1017
1018
1019
1020
1021
1022
1023
1024
1025
1026
1027
1028
1029
1030
1031
1032
1033
1034
1035
1036
1037
1038
1039
1040
1041
1042
1043
1044
1045
1046
1047
1048
1049
1050
1051
1052
1053
1054
1055
1056
1057
1058
1059
1060
1061
1062
1063
1064
1065
1066
1067
1068
1069
1070
1071
1072
1073
1074
1075
1076
1077
1078
1079
1080
1081
1082
1083
1084
1085
1086
1087
1088
1089
1090
1091
1092
1093
1094
1095
1096
1097
1098
1099
1100
1101
1102
1103
1104
1105
1106
1107
1108
1109
1110
1111
1112
1113
1114
1115
1116
1117
1118
1119
1120
1121
1122
1123
1124
1125
1126
1127
1128
1129
1130
1131
1132
1133
1134
1135
1136
1137
1138
1139
1140
1141
1142
1143
1144
1145
1146
1147
1148
1149
1150
1151
1152
1153
1154
1155
1156
1157
1158
1159
1160
1161
1162
1163
1164
1165
1166
1167
1168
1169
1170
1171
1172
1173
1174
1175
1176
1177
1178
1179
1180
1181
1182
1183
1184
1185
1186
1187
1188
1189
1190
1191
1192
1193
1194
1195
1196
1197
1198
1199
1200
1201
1202
1203
1204
1205
1206
1207
1208
1209
1210
1211
1212
1213
1214
1215
1216
1217
1218
1219
1220
1221
1222
1223
1224
1225
1226
1227
1228
1229
1230
1231
1232
1233
1234
1235
1236
1237
1238
1239
1240
1241
1242
1243
1244
1245
1246
1247
1248
1249
1250
1251
1252
1253
1254
1255
1256
1257
1258
1259
1260
1261
1262
1263
1264
1265
1266
1267
1268
1269
1270
1271
1272
1273
1274
1275
1276
1277
1278
1279
1280
1281
1282
1283
1284
1285
1286
1287
1288
1289
1290
1291
1292
1293
1294
1295
1296
1297
1298
1299
1300
1301
1302
1303
1304
1305
1306
1307
1308
1309
1310
1311
1312
1313
1314
1315
1316
1317
1318
1319
1320
1321
1322
1323
1324
1325
1326
1327
1328
1329
1330
1331
1332
1333
1334
1335
1336
1337
1338
1339
1340
1341
1342
1343
1344
1345
1346
1347
1348
1349
1350
1351
1352
1353
1354
1355
1356
1357
1358
1359
1360
1361
1362
1363
1364
1365
1366
1367
1368
1369
1370
1371
1372
1373
1374
1375
1376
1377
1378
1379
1380
1381
1382
1383
1384
1385
1386
1387
1388
1389
1390
1391
1392
1393
1394
1395
1396
1397
1398
1399
1400
1401
1402
1403
1404
1405
1406
1407
1408
1409
1410
1411
1412
1413
1414
1415
1416
1417
1418
1419
1420
1421
1422
1423
1424
1425
1426
1427
1428
1429
1430
1431
1432
1433
1434
1435
1436
1437
1438
1439
1440
1441
1442
1443
1444
1445
1446
1447
1448
1449
1450
1451
1452
1453
1454
1455
1456
1457
1458
1459
1460
1461
1462
1463
1464
1465
1466
1467
1468
1469
1470
1471
1472
1473
1474
1475
1476
1477
1478
1479
1480
1481
1482
1483
1484
1485
1486
1487
1488
1489
1490
1491
1492
1493
1494
1495
1496
1497
1498
1499
1500
1501
1502
1503
1504
1505
1506
1507
1508
1509
1510
1511
1512
1513
1514
1515
1516
1517
1518
1519
1520
1521
1522
1523
1524
1525
1526
1527
1528
1529
1530
1531
1532
1533
1534
1535
1536
1537
1538
1539
1540
1541
1542
1543
1544
1545
1546
1547
1548
1549
1550
1551
1552
1553
1554
1555
1556
1557
1558
1559
1560
1561
1562
1563
1564
1565
1566
1567
1568
1569
1570
1571
1572
1573
1574
1575
1576
1577
1578
1579
1580
1581
1582
1583
1584
1585
1586
1587
1588
1589
1590
1591
1592
1593
1594
1595
1596
1597
1598
1599
1600
1601
1602
1603
1604
1605
1606
1607
1608
1609
1610
1611
1612
1613
1614
1615
1616
1617
1618
1619
1620
1621
1622
1623
1624
1625
1626
1627
1628
1629
1630
1631
1632
1633
1634
1635
1636
1637
1638
1639
1640
1641
1642
1643
1644
1645
1646
1647
1648
1649
1650
1651
1652
1653
1654
1655
1656
1657
1658
1659
1660
1661
1662
1663
1664
1665
1666
1667
1668
1669
1670
1671
1672
1673
1674
1675
1676
1677
1678
1679
1680
1681
1682
1683
1684
1685
1686
1687
1688
1689
1690
1691
1692
1693
1694
1695
1696
1697
1698
1699
1700
1701
1702
1703
1704
1705
1706
1707
1708
1709
1710
1711
1712
1713
1714
1715
1716
1717
1718
1719
1720
1721
1722
1723
1724
1725
1726
1727
1728
1729
1730
1731
1732
1733
1734
1735
1736
1737
1738
1739
1740
1741
1742
1743
1744
1745
1746
1747
1748
1749
1750
1751
1752
1753
1754
1755
1756
1757
1758
1759
1760
1761
1762
1763
1764
1765
1766
1767
1768
1769
1770
1771
1772
1773
1774
1775
1776
1777
1778
1779
1780
1781
1782
1783
1784
1785
1786
1787
1788
1789
1790
1791
1792
1793
1794
1795
1796
1797
1798
1799
1800
1801
1802
1803
1804
1805
1806
1807
1808
1809
1810
1811
1812
1813
1814
1815
1816
1817
1818
1819
1820
1821
1822
1823
1824
1825
1826
1827
1828
1829
1830
1831
1832
1833
1834
1835
1836
1837
1838
1839
1840
1841
1842
1843
1844
1845
1846
1847
1848
1849
1850
1851
1852
1853
1854
1855
1856
1857
1858
1859
1860
1861
1862
1863
1864
1865
1866
1867
1868
1869
1870
1871
1872
1873
1874
1875
1876
1877
1878
1879
1880
1881
1882
1883
1884
1885
1886
1887
1888
1889
1890
1891
1892
1893
1894
1895
1896
1897
1898
1899
1900
1901
1902
1903
1904
1905
1906
1907
1908
1909
1910
1911
1912
1913
1914
1915
1916
1917
1918
1919
1920
1921
1922
1923
1924
1925
1926
1927
1928
1929
1930
1931
1932
1933
1934
1935
1936
1937
1938
1939
1940
1941
1942
1943
1944
1945
1946
1947
1948
1949
1950
1951
1952
1953
1954
1955
1956
1957
1958
1959
1960
1961
1962
1963
1964
1965
1966
1967
1968
1969
1970
1971
1972
1973
1974
1975
1976
1977
1978
1979
1980
1981
1982
1983
1984
1985
1986
1987
1988
1989
1990
1991
1992
1993
1994
1995
1996
1997
1998
1999
2000
2001
2002
2003
2004
2005
2006
2007
2008
2009
2010
2011
2012
2013
2014
2015
2016
2017
2018
2019
2020
2021
2022
2023
2024
2025
2026
2027
2028
2029
2030
2031
2032
2033
2034
2035
2036
2037
2038
2039
2040
2041
2042
2043
2044
2045
2046
2047
2048
2049
2050
2051
2052
2053
2054
2055
2056
2057
2058
2059
2060
2061
2062
2063
2064
2065
2066
2067
2068
2069
2070
2071
2072
2073
2074
2075
2076
2077
2078
2079
2080
2081
2082
2083
2084
2085
2086
2087
2088
2089
2090
2091
2092
2093
2094
2095
2096
2097
2098
2099
2100
2101
2102
2103
2104
2105
2106
2107
2108
2109
2110
2111
2112
2113
2114
2115
2116
2117
2118
2119
2120
2121
2122
2123
2124
2125
2126
2127
2128
2129
2130
2131
2132
2133
2134
2135
2136
2137
2138
2139
2140
2141
2142
2143
2144
2145
2146
2147
2148
2149
2150
2151
2152
2153
2154
2155
2156
2157
2158
2159
2160
2161
2162
2163
2164
2165
2166
2167
2168
2169
2170
2171
2172
2173
2174
2175
2176
2177
2178
2179
2180
2181
2182
2183
2184
2185
2186
2187
2188
2189
2190
2191
2192
2193

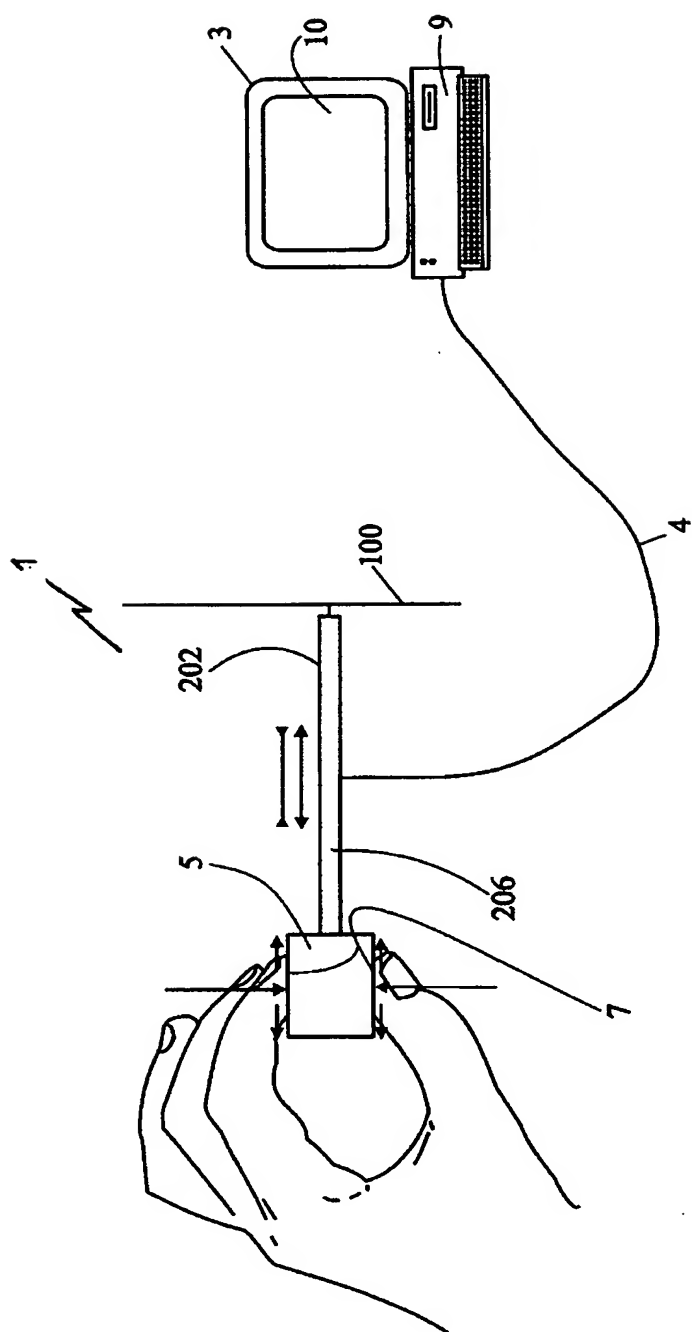


Figure 1

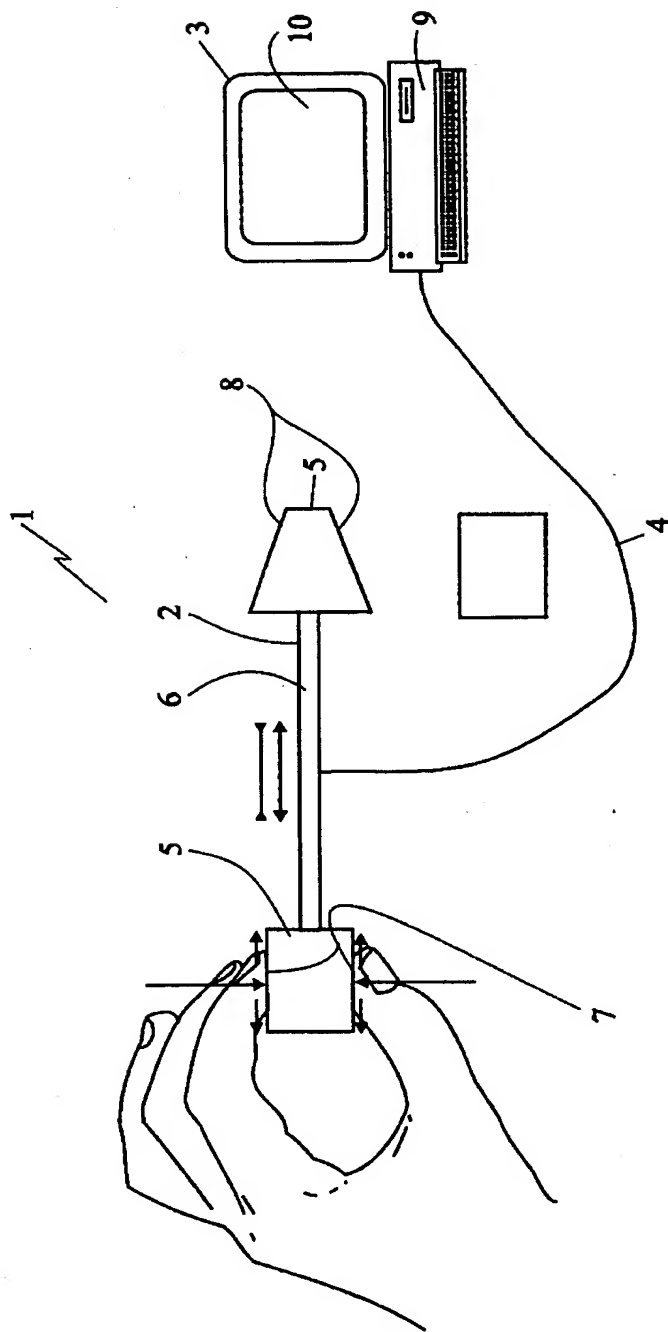


Figure 2

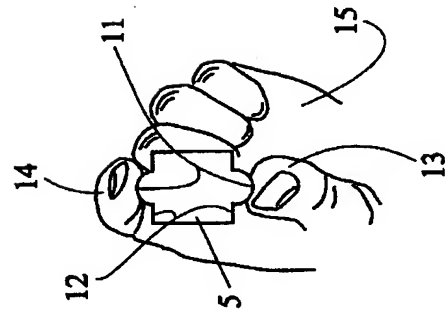


Figure 3

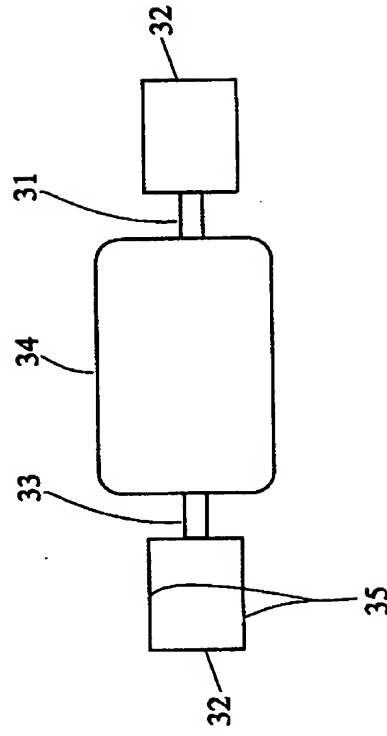


Figure 4

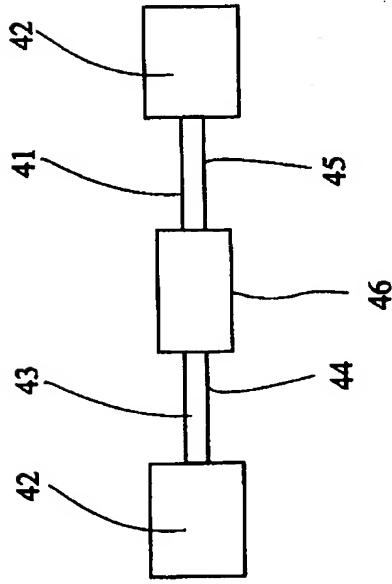


Figure 5

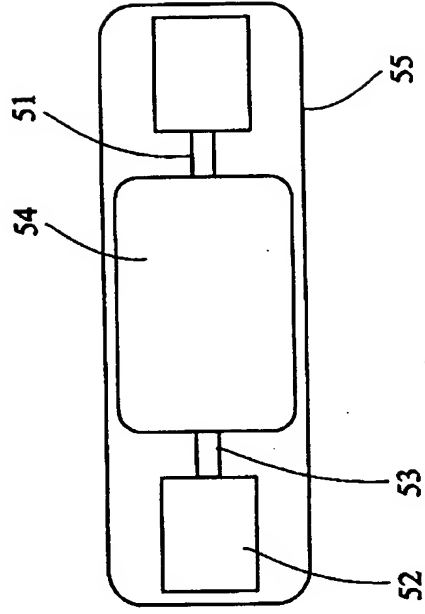
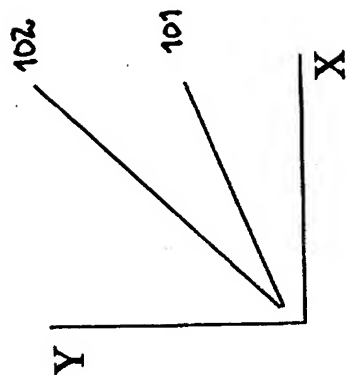
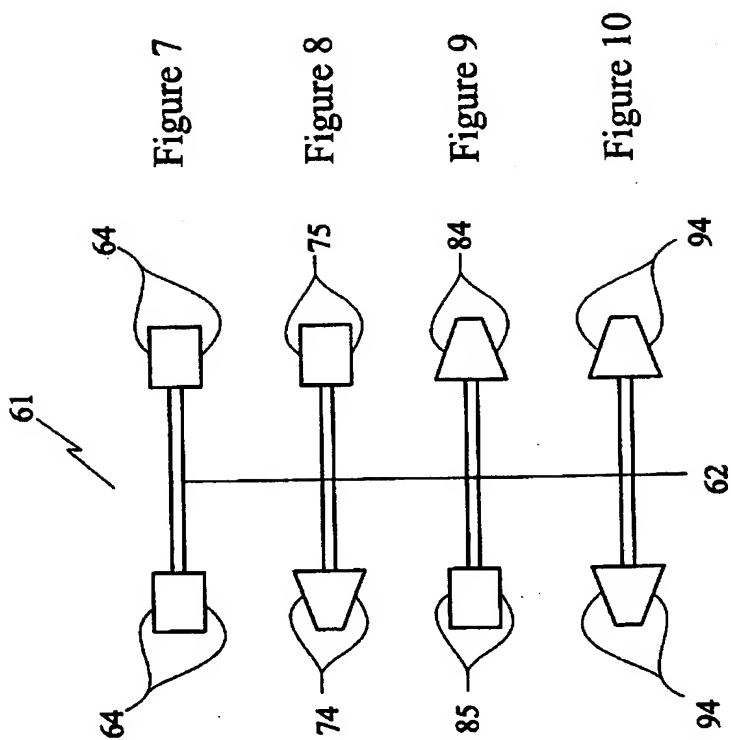


Figure 6

01032303-3

PR0010903



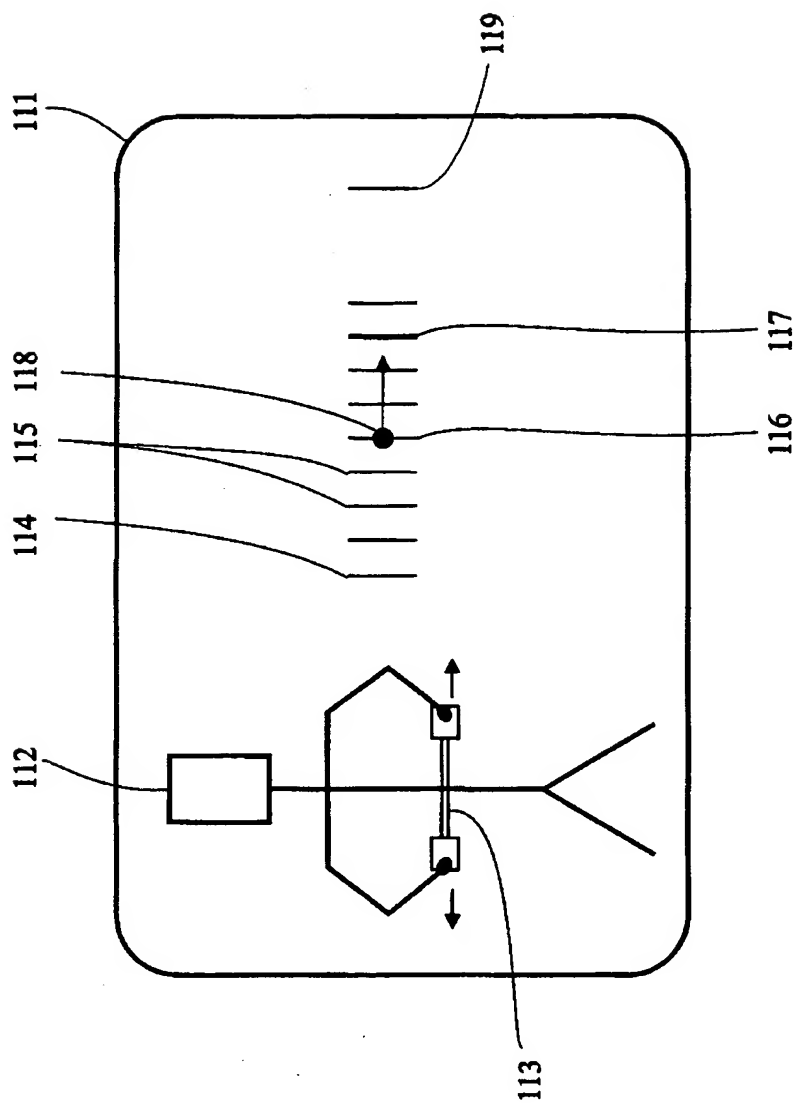


Figure 12